



MASTER Installation

The MASTER PC corresponds to that to which the AAG_CloudWatcher device is connected.

1. Run Setup.exe;
2. Create a directory in a local disk and make it shareable to other users in the local network;
3. Connect the AAG_CloudWatcher before starting the program;
4. Start program;
5. The program will prompt you




6. Select Yes for MASTER installation;
7. The program will display the following window:

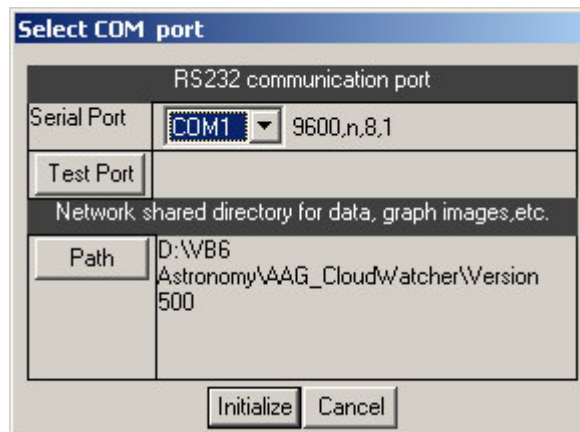


- Select the port number to which the AAG_CloudWatcher is connected and select the path corresponding to the directory in 2);
- Select button Initialize and the system will initialize the electrical constants for the device.

- The program will display Constants section of the Device TAB.

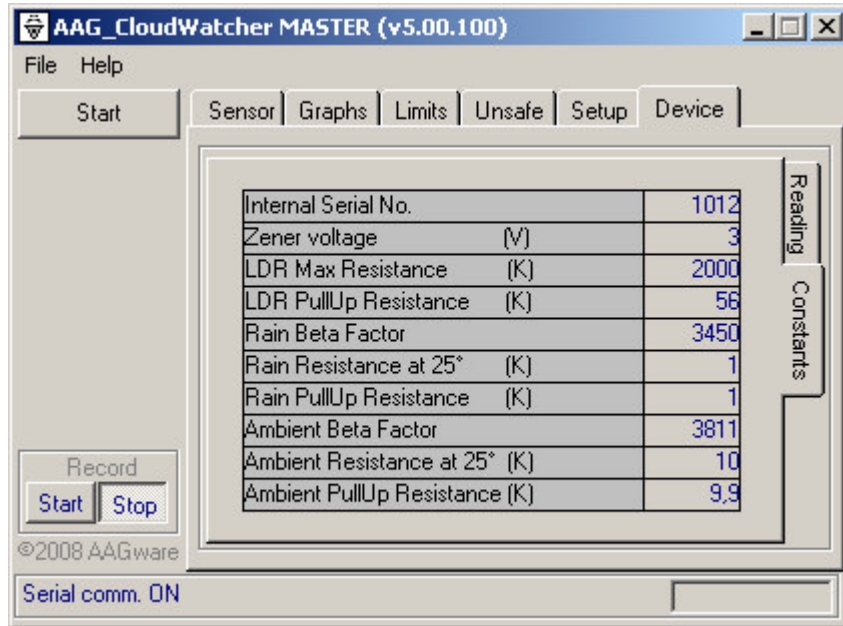

8. Check the Device section of the Setup TAB.

- Select *Switch Cntrl disabled* if you do not wish the AAG_CloudWatcher to control the switch - this allows other external programs to control the switch;
- Check the Temperature Correction Factors K1, K2, K3, K4 and K5 and do any adjustments that you deem necessary;



9. Check the Graph section of the Setup TAB.

- Adjust the graph time span by adjusting the number of points and frequency.
The total graph span is given by:
Total Span = (No. of Points) x (Frequency) x (Read Cycle)
- Use PNG image files rather than JPEG – they are smaller in size and have a higher quality;

